


Point Of Care Testing (POCT) Fully Automated Biochemistry Analyzer

SD1 auto dry biochemistry analyzer is a biochemical analysis system that integrates conventional biochemistry, coagulation, electrolyte and immunoassay items. it is widely used in primary health, emergency diagnostic testing, field rescue and other fields.









Equipped with the latest medical and technological innovations, we have invented a state-of-the-art portable SD1 auto dry biochemistry analyzer which provides a better, faster and more accurate diagnosis for blood analysis.





Test results in 12 minutes



3-step simple operation

ADVANTAGES

Low Sample Consumption

Sample Volume needed is 1/10 - 1/20 of conventional chemistry analyzer.

Easy to Use

No professional skill required.

Maintenance Free

Robust analyzer, no consumables needed, such as tubes, pumps and valves.

Accurate Result

Using the photoelectric colorimetric principle, the SD1 analyzer has many advantages versus conventional dry biochemistry analyzer using the light reflection method. Dilution of test sample is guaranteed without random errors or cross contamination.


SPECIFICATION

Sample volume:	100µl	Testing method:	End point, kinetic, fixed time, turbidmetry etc					
Bar code:	QR code							
Testing time:	12 minutes / sample	Light source:	12V/20W, Halogen tungsten lamp with life span over 2500 hours					
Temperature:	37℃±0.3℃	Power supply:	AC 100V-240V, 50-60Hz					
Resolution:	0.001Abs	Power:	Output: 15 🛲 7.0a, 105W MAX					
Absorbance:	0-3.0Abs	rower.	Android 7.0 inch 800*480, multi-point capacitive touch screen, multilingual choice					
Sample type:	Anti-coagulation whole blood, serum, plasma	Display:						
	Temperature:10-30°C Humidity: 30%-70%	Storage:	500,000 results					
Work condition:		Printer:	Built-in thermal printer					
Testing principle:	Absorption spectroscopy,	THINEI.						
	transmission turbidimetry	Interface:	4 USB ports, 1 LAN port					
QC&Calibration:	IQC (Intelligent Quality Control)	Dimension:	315*375*475mm. 4.2kg(N.W.), 7kg(G.W.)					



EASY 3-STEP OPERATION

All steps are automated from centrifugation, dilution, quality control to test result printing.

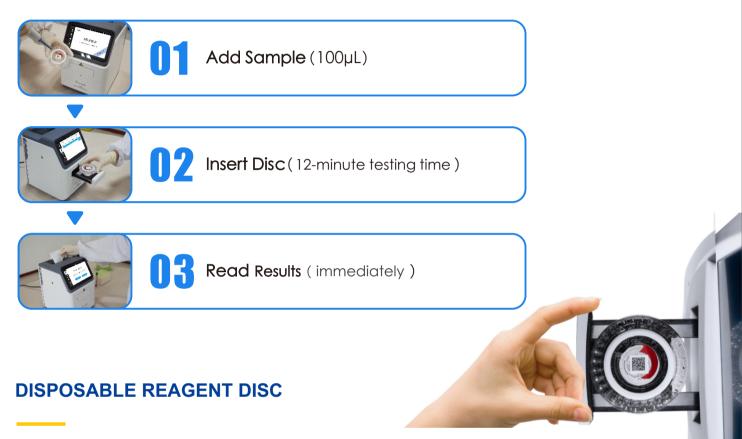

Seamaty Reagent Disc Introduction

Born from space technology research, Seamaty reagent disc is a fully self-contained single-use chemistry reagent disc designed to satisfy a variety of conditions. Just 3-4 drops (100μ I) of whole blood are required to offer accurate results. The test kit consists of lyophilized reagent beads, diluent and QR code. The reagent disc has a shelf life of 12 months(2-8°C storage). The diluent is contained in the disc. The QR code includes the basic information of the disc.

Intelligent Quality Control

The reagent disc contains a complicated internal quality control system IQC which continuously monitors the disc function to ensure reaction stability and optimal disc performance. IQC is the engine that drives the SD1 accurately and precisely.

Correlation

In countless central-lab correlation studies, the accuracy, precision and reproducibility of the SD1 chemistry analyzer has been proven and approved by the most respected hospitals, clinics and laboratories around the world.

Reagent Panel

Group Panels		General Chemistry II Kit							General Chemistry III Kit										
	8 Renal Function Kit	7 Electrolyte Kit	4 Cardiac Kit	10 Relyte	18 General Chemistry II Kit	8 Renal Function Kit	7 Relyte Kit	14 General Chemistry Kit	10 Liver Function	6 Lipid	19 General ChemistryIII Kit	10 Liver Function	10 Livernal Function	13 Health Check Kit		al 14 General Chemistry B Kit	l 11 Chemistry CRP Kit	5 CRP Kit	
Analytes	`	Kit AW00246		Kit MD20105	Kit AW00866			кіт AW00002	Kit AW00131	Kit AW0035	Kit 3 AW00867	Pius Kit AW00430	кіт AW01078	AW00194			CRP Kit AW00857		
ALB	ALB				ALB	ALB		ALB	ALB		ALB	ALB	ALB	ALB	ALB	ALB	ALB		
ALP								ALP	ALP		ALP	ALP	ALP		ALP		ALP		
ALT								ALT	ALT	ALT	ALT	ALT	ALT	ALT	ALT	ALT	ALT		
AMY					AMY			AMY	AMY		AMY	AMY		AMY		AMY		AM	
AST			AST		AST			AST	AST	AST	AST	AST	AST	AST	AST	AST	AST		
Са	Ca	Ca		Ca	Ca	Са								Ca					
CHE									CHE		CHE		CHE		CHE				
СК			СК		СК						СК			СК		СК			
Cl		Cl⁻		Cl⁻	Cl⁻	Cl⁻	Cl⁻												
Crea	Crea			Crea	Crea	Crea	Crea	Crea			Crea		Crea	Crea	Crea	Crea	Crea	Cree	
DB											DB	DB	DB		DB	DB	DB		
GGT								GGT	GGT		GGT	GGT	GGT		GGT				
GLU	GLU				GLU		GLU	GLU		GLU	GLU			GLU	GLU	GLU	GLU		
K+		K⁺		K+	K⁺	K⁺	K+												
Na+		Na⁺		Na+	Na⁺	Na⁺	Na+												
PHOS	PHOS	PHOS		PHOS	PHOS									PHOS					
TB								TB	TB		TB	TB	TB	TB	TB	ТВ	ТВ		
TBA									TBA		TBA		TBA		TBA				
tCO ₂	†CO2	tCO ₂		†CO2	tCO ₂		†CO2												
TP								TP	TP		TP	TP	TP	TP	TP	TP	TP		
UA	UA			UA	UA	UA		UA			UA		UA		UA	UA			
UREA	UREA			UREA	UREA	UREA	UREA	UREA			UREA		UREA	UREA	UREA	UREA	UREA	URE/	
TC								TC		TC	TC				TC	TC			
TG								TG		TG	TG			TG	TG	TG			
HDL										HDL	HDL				HDL				
LDL*										LDL*	LDL*				LDL*				
LPS					LPS							LPS						LPS	
HBDH			HBDH		HBDH														
LDH			LDH		LDH														
CRP																	CRP	CRI	
Mg		Mg		Mg	Mg														
GLOB*								GLOB*	GLOB*		GLOB*	GLOB*	GLOB*	GLOB*	GLOB*	GLOB*	GLOB*		
U/C*	U/C*			U/C*	U/C*	U/C*	U/C*	U/C*			U/C*		U/C*	U/C*	U/C*	U/C*	U/C*		
A/G*								A/G*	A/G*		A/G*	A/G*	A/G*	A/G*	A/G*	A/G*	A/G*		

* calculated